

Operation manual

# Krypton K

Measuring system for monitoring and control of the concentration of total Chlorine





**DR. A. KUNTZE**

GUTES WASSER MIT SYSTEM

Dr. A. Kuntze GmbH  
Robert-Bosch-Str. 7a  
D-40668 Meerbusch  
Tel. +49-21 50-70 66-0  
Fax +49-21 50-70 66-60  
info@kuntze.com  
www.kuntze.com

---

# Contents

<b>1. Your Krypton K</b> .....	<b>4</b>
1.1 General and Safety instructions .....	5
1.2 Application .....	6
1.3 Intended use .....	6
1.4 Features .....	7
1.5 Technical data .....	8
<b>2. Installation</b> .....	<b>9</b>
2.1 Set up .....	10
2.2 Connection diagram .....	11
2.3 Installation procedure .....	12
<b>3. Operation of the instrument</b> .....	<b>13</b>
3.1 How to adjust parameters .....	14
3.2 Menu overview .....	15
<b>4. Password and language</b> .....	<b>16</b>
<b>5. Adjustment of the meter</b> .....	<b>17</b>
5.1 Calibration .....	18
5.2 Averaging .....	18
5.3 Temperature compensation .....	19
<b>6. Adjustments of the controller</b> .....	<b>20</b>
6.1 ON/OFF controller .....	21
6.2 P / PI controller as impulse-frequency controller .....	22
6.3 P / PI controller as pulse-pause controller .....	23
6.4 Activation and deactivation of the controller .....	24
6.5 Turn-on delay .....	24
6.6 External controller stop .....	24
6.7 Manual operation of the relays .....	25
6.8 Limit values and Alarm .....	26
6.9 Dosage check .....	27
<b>7. Data output</b> .....	<b>28</b>
7.1 Current output .....	28
7.2 Serial interface RS485 .....	28
<b>8. Operation and maintenance</b> .....	<b>29</b>
<b>9. Service</b> .....	<b>31</b>
9.1 Product info .....	31
9.2 Analog inputs .....	31
9.3 Erase settings (reset) .....	31
<b>10. Error messages</b> .....	<b>32</b>
<b>Index</b> .....	<b>33</b>
<b>Customer settings - for reference!</b> .....	<b>35</b>

## **1. Your Krypton K**

is a product by Dr.A. Kuntze GmbH, Germany that offers high quality and reliability for years.

The system is delivered ready-to-use, all mounted on a board, with a pre-adjusted working potential suitable for your measurement. It is even pre-calibrated, so you will receive approximate measured values immediately after installation. Single-point calibration is used to determine the electrode's response characteristic.

The Krypton K's instrument K 100 has two integrated controllers which provides bidirectional PI control, via two relays or as a steady-state controller via the analog output. You can define a turn-on delay to prevent wrong dosage after power failure and operate the controller by remote control. A flow monitor will stop the controllers automatically in a low water situation. Activate dosage check to get an alarm if dosage achieves no results, indicating damages in the feeding lines.

Let's not forget the alarm function with minimum and maximum limit and turn-on delay...

You have certainly made a good choice. On the following pages you learn more about your Krypton K. If, however, you have further questions or are looking for information not included in this manual or if you are interested in supplementing products like sensors or armatures or in our other instrument series, just give us a call - we will be delighted to help you!

## **1.1 General and Safety instructions**

This manual applies to the following instruments:

<b>Instrument and type</b>	<b>Revision date</b>
Krypton K SCI <sub>2</sub>	12/08

It contains technical information for the installation, start-up and maintenance. If you have any questions not included in this manual please contact your supplier or the official representative of Dr. A. Kuntze GmbH in your country.

We would like to point out that the warranties specified in our general trading conditions are valid only if

- installation, connections, adjustments, start-up, and maintenance of the instrument are carried out by authorized personnel with adequate qualification.
- the instrument is used according to the description in this manual.

Please check for damages immediately after receiving the instruments and report any damages within 24 hours to the delivering company. Never work with a damaged instrument.

Keep this manual at a safe place where you can always look up the safety instructions and the informations on handling and usage. According to DIN 61010 the manual is part of the product and must be maintained as long as the instrument is used, and given to the next owner if the instrument is sold.

This instrument was designed and built according to the safety measures for electronic devices and has left our company in perfect working condition. To preserve this condition and to ensure safe usage follow all instructions carefully and pay special attention to all warnings issued in this manual. If the instrument is visibly damaged or has been stored inappropriately or if there are any doubts concerning safe usage, shut it down and make sure it cannot be restarted by accident.

You will notice that important safety instructions are highlighted:

- WARNING** highlights instructions for the protection of people. Disregarding these instructions may cause accidents and injuries!
- ATTENTION** highlights instructions for the protection of the instrument and the equipment. Disregarding these instructions may lead to damage or destruction of the instrument or equipment!
- NOTE** is used to highlight interesting details.

## **1.2 Application**

Krypton K SCI2 systems are used to measure the concentration of total Chlorine, which is the sum of free Chlorine and organically bound Chlorine. They have integrated controllers to operate actuators such as dosing pumps or valves to add chemicals until the desired concentration is reached and maintained.

Applications are detoxication of industrial waste water, water treatment, and disinfection.

While the controller is set to Automatic, it controls independently the dosing of possibly hazardous chemicals, according to the measured values.

For safety measures, both the measurement and the calibration are checked for failure. Failures are indicated in the display and via the alarm relay, which can set off a horn or lamp or relate to a central control. If that failure makes control unreliable, the controller is automatically switched off until the failure has been taken care off.

**CAUTION**     **The instrument checks the input signals, the calibration results, and the water flow. It cannot detect erroneous settings or failures in the treatment system, nor can it check for plausibility! The safety of the system of which the instrument is part of, lies within the reach of responsibility of whoever built the system.**

## **1.3 Intended use**

Use these instruments only for the monitoring and control of water.

Use only sensors, assemblies, and accessories of Dr. A. Kuntze, since instruments and sensors are attuned.

Ensure that the required measuring conditions are constantly maintained, such as flow, pressure, temperature, etc.

Set-up the instrument according to this manual. Carry out all the steps described, and check all measurements and settings before you activate the controller.

Use all available safety measures such as the alarm relay, the dosage check, and the lack-of-water indication.

Regularly check that all safety measures are in good working order.

**CAUTION**     **The protection built into the instrument is impaired if they are not used as intended!**

---

## **1.4 Features**

### **Meter**

Measuring ranges	0.00 - 10.00 mg/l Total Chlorine as Cl <sub>2</sub> -30.0 - 140.0 °C
Display	Measured value and temperature with dimension Status display sensor, calibration, controller & alarm
Temperature compensation	manual or automatic with Pt100
Calibration	1-point calibration; zero-point-calibration possible
Averaging	can be activated and deactivated via menu

### **Controller**

Set points	2 set points with adjustable direction
Controller types	ON/OFF controller with hysteresis P controller as Pulse-Pause-, Impulse-Frequency- or steady controller PI controller as Pulse-Pause-, Impulse-Frequency- or steady controller
Hysteresis	adjustable within the measuring range
P range X <sub>p</sub>	adjustable within the measuring range
Integral time T <sub>N</sub>	0 - 2000 sec.
Least pulse	0.1 - 9.9 sec.
Pulse+Pause time	02 - 99 sec.
Impulse frequency	100 - 7200 pulses/h
Turn-on delay	0 - 200 sec.
Dosage check	0 - 90 min
Alarm function	min. and max. limit and onset delay

### **Connections**

Relays	3 potential-free contacts (2x controller, 1x alarm) 6 A, 250 V, max. 550 VA
Analog outputs	0/4-20 mA galvanically isolated, max. loading 500 Ohm +/- 6V DC power supply for Total Chlorine sensor
Analog inputs	1 measuring input for Total Chlorine sensor 1 measuring input for temperature sensor
Digital input	external controller stop or low water indication
Serial interface	RS485, Baud rate 9600, data format 8Bit, 1start and 1stop bit, no parity

## **1.5 Technical data**

<b>Feature</b>	<b>Description</b>
Dimensions	400 x 700 x 90 mm (W x H x D)
Weight	4.2 kg
Terminals	spring terminals max. 1.5mm <sup>2</sup>
Protection class	IP 65
Power supply	230 V +6/-10%, 40 .. 60 Hz, optional 117 V or 24 V
Internal fuse	230 V: 63 mA HRC 117V : 125 mA HRC 24 V: 800 mA NRC
Power consumption	10 VA
Display	LCD, 2-line, 2x16 characters, illuminated background measured value and temperature with dimensions indication of relay status
Current output	0/4-20 mA, galvanically isolated, max. loading 500 Ohm
Interface	RS485, Baud rate 9600, Data formate 8Bit, 1 Start / 1 Stop bit
Controller	ON/OFF controller with hysteresis, P or PI controller as Pulse-Pause- or Impulse-frequency controller, steady controller, bidirectional PI control action, adjustable onset-delay, manual operation of the relays, controller stop via external switch or level sensor (lack-of-water sensor)
Set points	2 set points adjustable within the measuring range
Alarm function	with min. and max. limit and turn-on delay
Contact rating	6 A/ 250 V, max. 550 VA resistive load (with RC protective circuit)
Operation temperature	0 - 50°C
Storage temperature	-20 - 65°C
Humidity	max. 90% at 40°C non-condensing

## 2. Installation

The measuring system is delivered ready-to-use. All you have to do is mount it on a suitable wall, install the sensors, and connect the water inlet and outlet. The positions of the sensors are shown on the next page.

**ATTENTION** Install the instrument in a place where it is not put under mechanical or chemical strain!

Mind the protection class: IP65 (closed terminal cover)

**ATTENTION** The membrane sensor is delivered with empty membrane-cap. Do the filling and set-up according to the sensor's manual.

### Connections:

You will find a detailed connection diagram on the following pages.


Before connecting the power supply check the information on the instrument label.

**ATTENTION** Input, output and control lines must be installed separate from each other and separate from power lines!

For inputs and outputs use screened cables, and connect the screens on one side only.

To protect the measurements against interferences use only the special cables delivered for each measurement.

When using the relays, mind that with inductive loads, interference must be suppressed. If that is not possible, the relay must be protected at the terminals of the dialog by a resistance-capacitance filter, or, in case of direct current, by a free-wheeling diode.

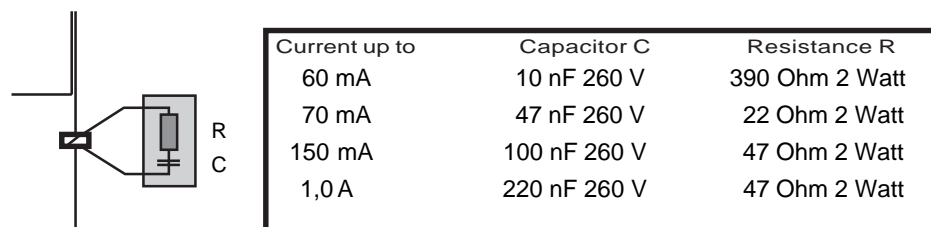

### Tube connections:

Connect the water inlet on the left side and the outlet on the right side of the flow cell. Water must be supplied at 30-300, ideally 50-200l/h. The outlet has to be an open outlet, pressureless, or at least with a pressure under 1 bar.

## 2.1 Set up



- 1 Meter / controller  
K 100 W
- 2 Water inlet
- 3 Flow monitor with  
integrated Pt100
- 4 Sampling point
- 5 Total Chlorine sensor
- 6 Water outlet


### **Sensors:**

Flow&temperature sensor      PT-55-W

Total Chlorine measurement      CP2.1N

**ATTENTION** The membrane sensor is delivered with empty membrane-cap. For filling and set-up please refer to the sensor manual.

## 2.2 Connection diagram

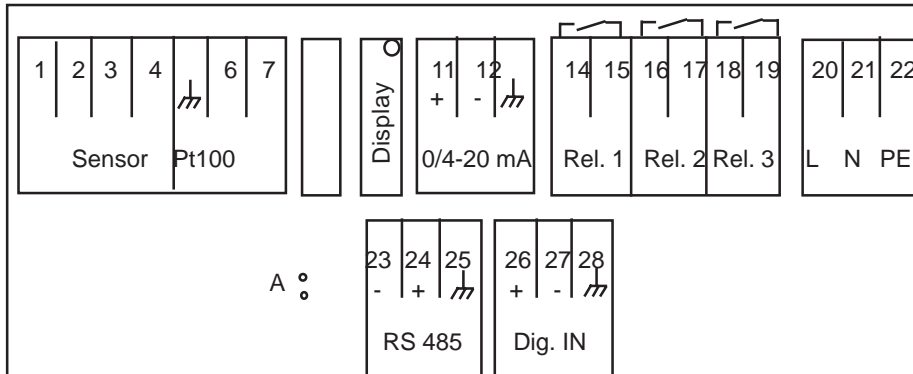

Connection	Terminal	Notes
Total Chlorine Sensor	1 - 4	1 + 2 = measurement 1 = yellow, 2 = green 3 + 4 = power supply sensor 3 = -6V = white, 4 = +6V = brown
Flow monitor /Pt100	6 + 7 26 + 27	PT100, brown + white flow monitor, blue + black
Display contrast	Display	Potentiometer to adjust the display contrast
Analog output	11 + 12	11 = +, 12 = -, maximum load 500 Ohm
Relay 1	14 + 15	
Relay 2	16 + 17	
Relay 3	18 + 19	Alarm relay
Power supply	20 + 21 + 22	Check information on the instrument label!
RS485 (Option)	23 + 24	23 = -, 24 = + Jumper A bridged = terminating impedance
Digital input	26 + 27	external controller stop

## **2.3 Installation procedure**

**ATTENTION** The membrane sensor is delivered with an empty membrane-cap. It has to be filled prior to measurements. Please refer to the sensor's manual for set-up and handling!

Mount the board on a suitable wall. Keep the water pipes going to the flow cell as short as possible.

**NOTE** For good control results the measured water has to be representative for the water that is to be controlled. Do not place the measurement directly after the injection points, make sure that the chemicals had time to mix properly with the water and keep all distances short to reduce delay times.

Take the sensors out of their boxes and prepare the membrane sensor according to the sensor's manual. Mount the sensors in the appointed slots and connect the cables according to their labels. Mind the height of the membrane sensor as shown in the sensor's manual. It must not block the water flow but low enough so that the outer metal ring is completely covered with water.

Connect the water inlet and outlet. Make sure that the outlet valve is open and the stop-cock at the bottom of the flow cell is closed.

Open the inlet valve slowly until the water flows through the flow cell with the desired flow rate.


Switch on the power supply for the instrument..

Wait a few minutes until all readings are stable. If air bubbles have got caught under the membrane sensor, remove them by careful movement of the sensor.

For calibration and settings follow the steps described in this manual.

**NOTE** Measurements with membrane sensors should be recalibrated after 24h, since their signal output often changes slightly over the first day.

## 3. Operation of the instrument

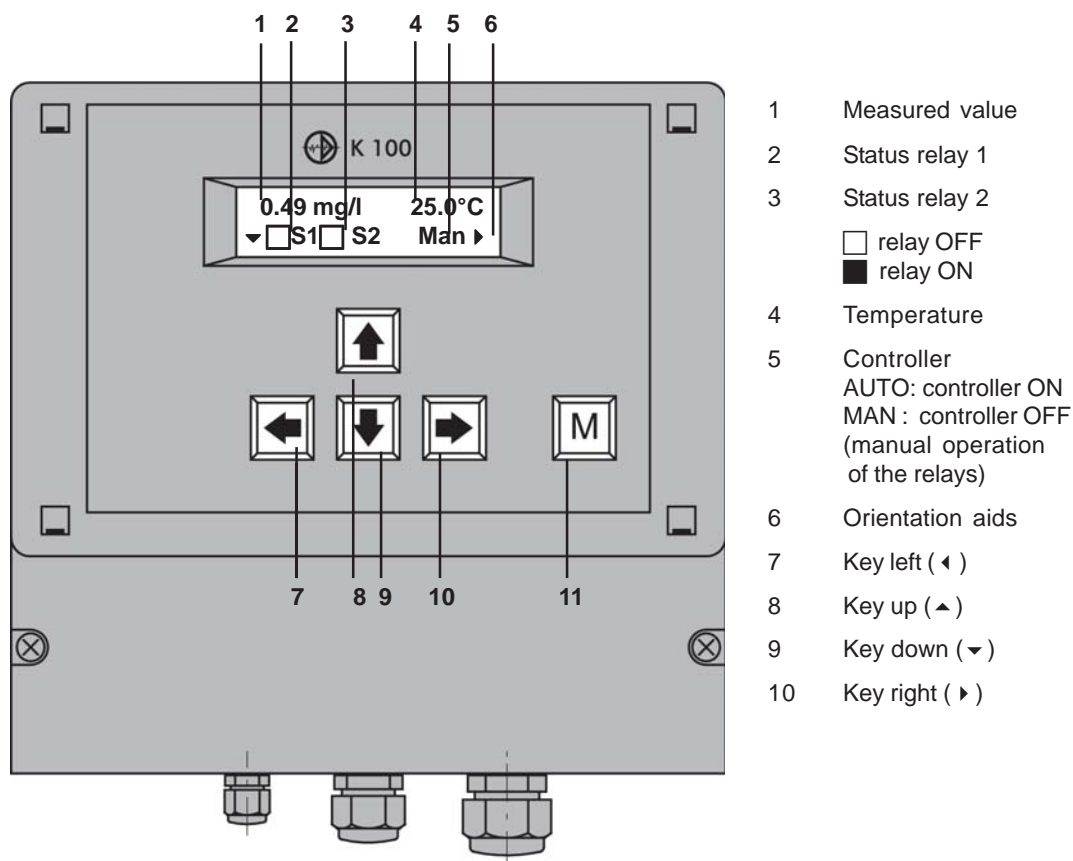

When turned on the instrument shows the measured value and temperature together with the controller mode (Man) and the status of the relays S1 and S2 (both OFF).

With five membrane keys you can move within the menu:

With key ▼ you enter the main menu.

With keys ▲ and ▼ you move up and down in the menu.

With key ▶ you address a menu or parameter.

With key ◀ you leave a menu or store a change.

For your convenience triangles in the display indicate the directions you can take from your position in the menu.

With key „M“ you get back to the display of the measured values from any point in the menu. Changes that have not been stored will be lost.

### 3.1 How to adjust parameters

Temp. Comp.  
▶ Manual Comp.

1) When you address a parameter the actual setting is displayed.

2) Switch to the next alternative setting with key ▶ .

Temp. Comp.  
▶ Automat. Comp.

3) When you have come to the last alternative, pressing the key once more will bring you back to the start.

Temp. Comp.  
▶ Manual Comp.

### Selection between alternatives

For many parameters you have the choice between two or more alternatives, for e. g. between manual and automatic temperature compensation. For these parameters you need only key ▶ . Switch from one alternative to the next until you either come back to where you started or until you reach the alternative you were looking for.

With these parameters any changes are immediately valid - there is no need to store the change.

Enter password  
▶ 058 Code

1) Address the parameter with key ▶ .

2) A double triangle appears behind the number indicating that the number can be changed now with keys ▲ and ▼ .

Enter password  
◀ 058 ◆ Code

3) Store the new value with key ◀ . The double triangle disappears - the new value is stored.

Enter password  
▶ 062 Code

### Adjustment of numerical parameters


Numerical parameters can only be altered when a double triangle is visible behind the number. This double triangle appears when you address the parameter with key ▶ .

Adjust the parameter with keys ▲ and ▼ . A short pressure on the key changes the last decimal by 1. If you keep the key pressed, the value will continue changing until the pressure is released.

Store the changes with key ◀ . The double triangle disappears.

**NOTE** If you do not want to store the change, press key „M“ instead of key ◀ .

## 3.2 Menu overview

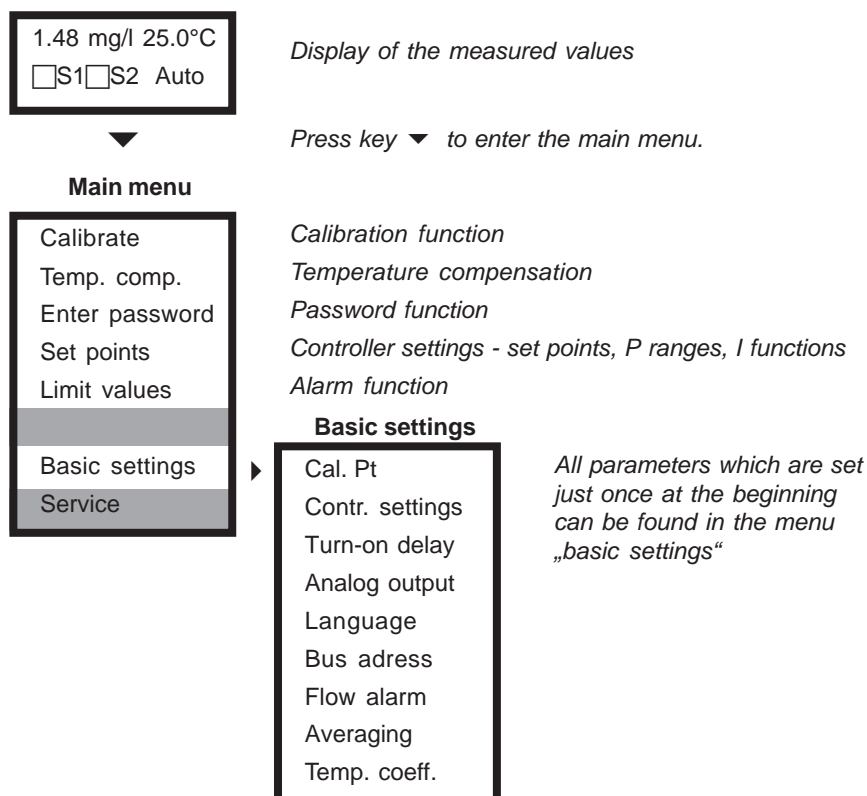


## Main menu and basic settings

The parameters are sorted into two menus: In the main menu you will find all functions which are used regularly, such as calibration. The menu basic settings contains all parameters which are set just once during start-up.

On the following pages you will find information on how to adjust parameters and which parameters you need for which application, in the following order:

- 1) General adjustments: password and language
- 2) Adjustments for measurement: calibration, temperature compensation, and averaging
- 3) Adjustments of the controller: selection of the controller version and corresponding parameters
- 4) Adjustments to read out data: analog, digitally and/or as alarm

## 4. Password and language

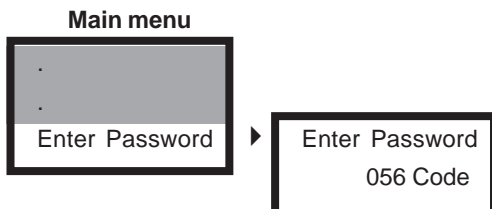


### Enter password

To get access to the various parameters you have to enter the correct password:

Code 11 gives access to the parameters „calibration“, „temperature compensation“, and „set points“.

Code 86 gives access to all parameters and functions.

With any other number it is impossible to select, view or change any parameter.

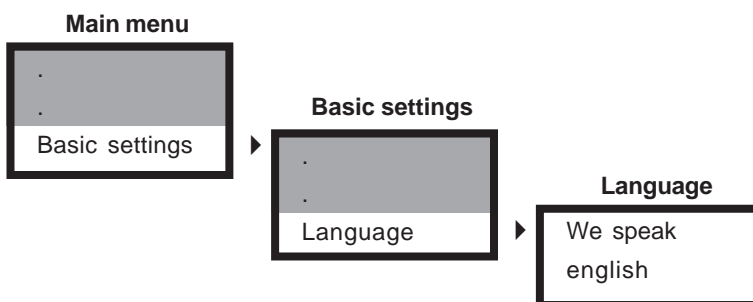


### Language

For the communication with the instrument you can choose from a variety of languages.

Since choosing a language is part of the basic settings, it requires code 86. If a different code is set, you will be asked to enter the correct password.

## 5. Adjustment of the meter

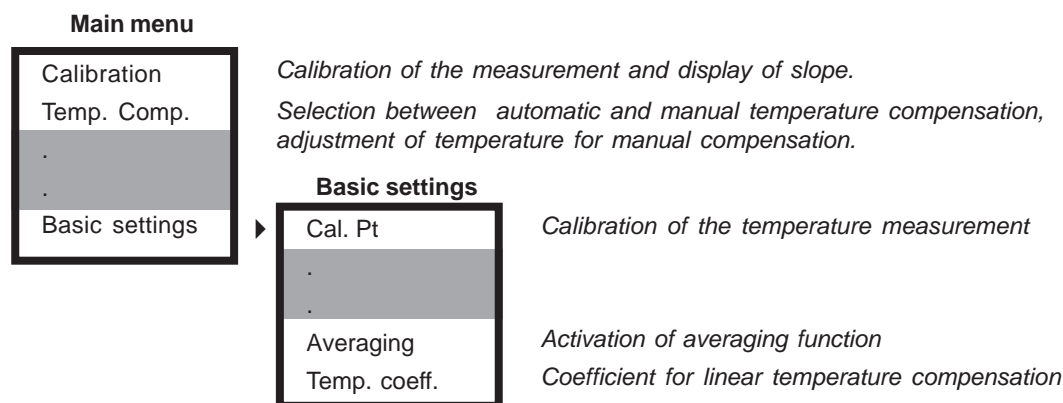

Potentiostatic measurements require a 1-point calibration:


Since the measurement depends upon the flow-rate and calibration solutions would not be stable anyway, the sensor cannot be taken out of the armature for calibration, as is done with pH sensors. Instead the actual concentration of the test water is determined by an alternative method, for example photometrically with DPD, and this value is entered as calibration value.

Zero-calibration is possible, too, if necessary.

The measurement is influenced by temperature. This influence can be compensated manually or automatically. For manual compensation the temperature is entered manually, for automatic compensation temperature has to be measured with a temperature sensor. For the temperature compensation a linear coefficient can be adjusted as %/K.

For smoother measured values activate the averaging function.


## 5.1 Calibration

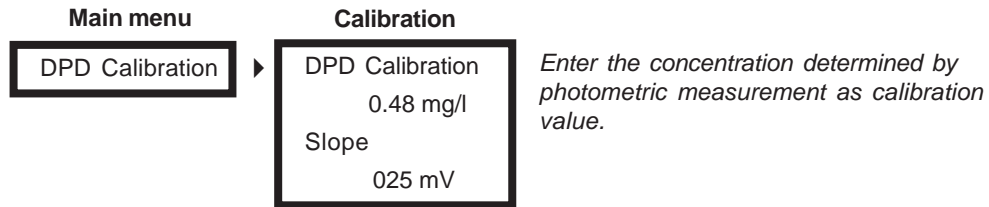

### Calibration of the measurement

- 1) Switch off the controller. Take a sample of the test water at the sampling point and determine the concentration by photometric DPD measurement or a similar reference method.
- 2) Enter the determined concentration and calibrate by pressing keys ▶ and ◀ : Start with key ▶ and then - while still applying pressure on this key - additionally press key ◀ .
- 3) Check the displayed slope before switching on the controller.


If you enter 0.00mg/l as calibration value, the instrument stores the signal automatically as zero-point.

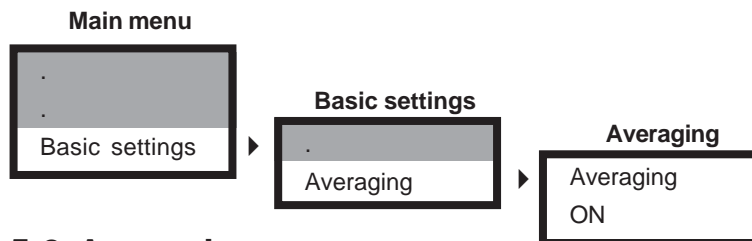

## 5.2 Averaging

In the basic settings you can activate an averaging function to smoothen the signals. This is especially useful when using membrane sensors.

## 5.3 Temperature compensation

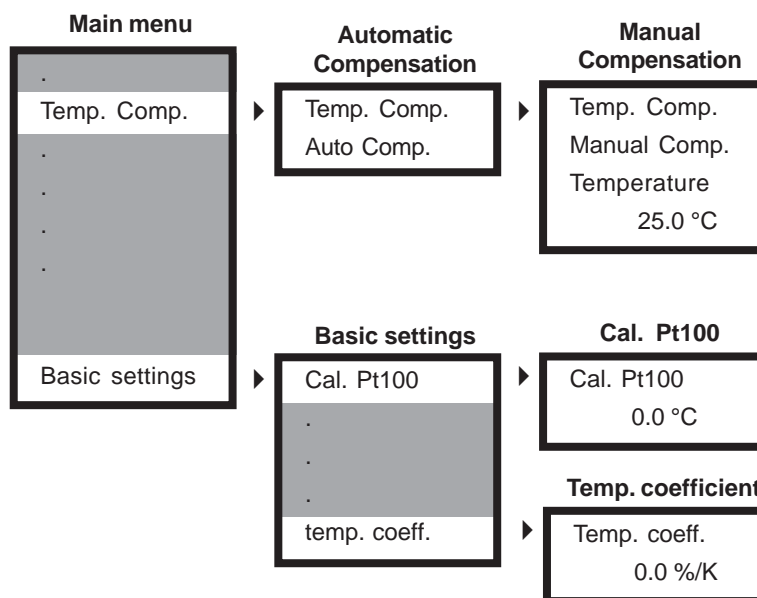

Choose between two types of temperature compensation:

- 1) Automatic compensation with temperature sensor

Mind that the temperature sensor should measure the temperature in the vicinity of the sensor. If temperature sensor and potentiostatic sensor are not immersed in the same solution, better switch to manual compensation.

- 2) Manual compensation

If the temperature is more or less stable you can enter it manually. The instrument will then compensate the temperature effect of this temperature.

### Temperature coefficient


With the temperature coefficient you can adjust the degree of compensation. The coefficient is given as %/K. For example, with a coefficient of 2%/K two percent of the measured value are subtracted per degree of temperature above 25°C.

### Calibration of the temperature measurement

Since the temperature sensor is connected with a twin-core cable, slight deviations might occur between measured and real temperature. These deviations can be eliminated by calibration.

During start-up, measure the temperature manually and enter a correction term so that the display shows the exact temperature.

## **6. Adjustments of the controller**

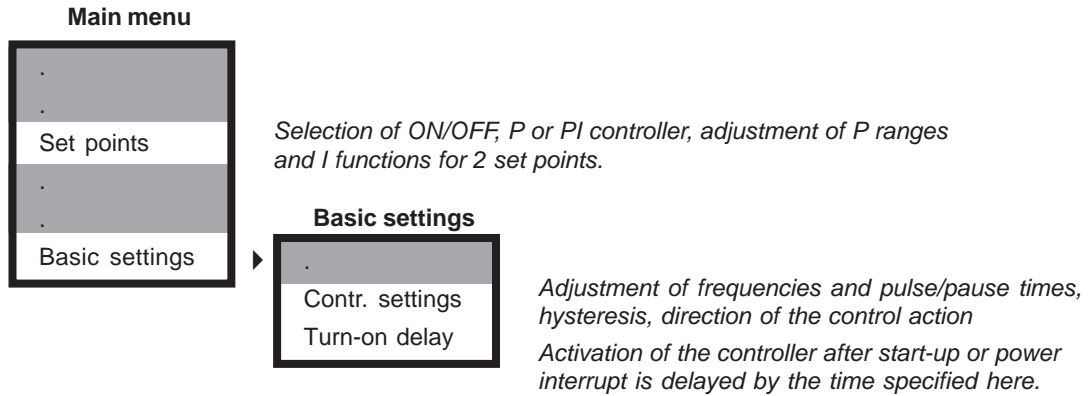

For any type of controller you have to enter one or two set points, and you have to tell the instrument whether these set points are reached by increasing or decreasing the measured value.

You can choose between three different controller versions:

### **ON/OFF controller**

The ON/OFF controller switches ON if the measured value exceeds the set point and OFF if it drops back below it or vice versa. Dosage is always carried out with 100% (ON) or 0% (OFF). The parameter for an ON/OFF controller is the hysteresis.


### **P controller**

The P controller or proportional controller reduces the dosage in the vicinity of the set point proportional to the control deviation. This is easily achieved if the analog output is used as steady control output. If the relays are used, the proportional reduction is achieved by either reducing the switch frequency (Impulse-frequency controller) or reducing the time within a given period of time in which the relay is ON (pulse-pause controller). The parameters for a P controller are the P range and the impulse-frequency or the pulse+pause time and the minimum pulse.

### **PI controller**

The PI controller is a P controller with an additional I function. Adjustments and parameters are the same as for an P controller. Additionally the integral action time has to be adjusted which determines the I function. The I function eliminates the P controller's disadvantage of a remaining steady-state deviation.

## 6.1 ON/OFF controller

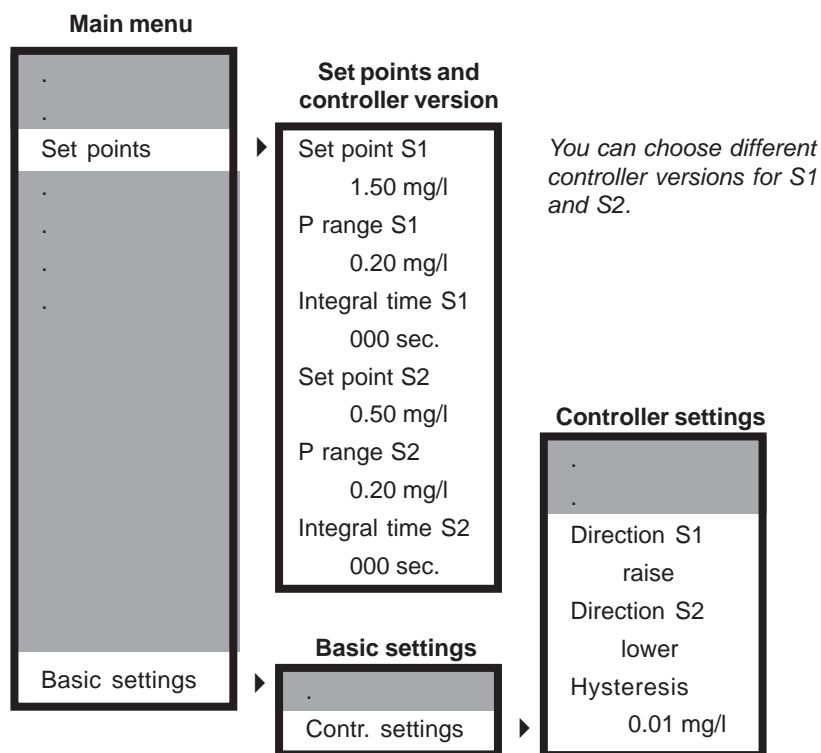

For an ON/OFF controller you have to set the following parameters:

### 1) Set points S1 and S2

Set point S1 refers to relay 1, set point S2 refers to relay 2.

### 2) P range and integral action time for S1 and S2

For an ON/OFF controller set P range = 0 and integral time = 0.


### 3) Acting direction for S1 and S2

Select „raise“ if the dosage raises the measured value.  
Select „lower“ if the dosage lowers the measured value.

### 4) optionally a hysteresis

The hysteresis prevents fast switching in the vicinity of the set point. If hysteresis is activated (by setting a value > 0) the relay switches only when the set point is exceeded by half the hysteresis.

## 6.2 P / PI controller as impulse-frequency controller

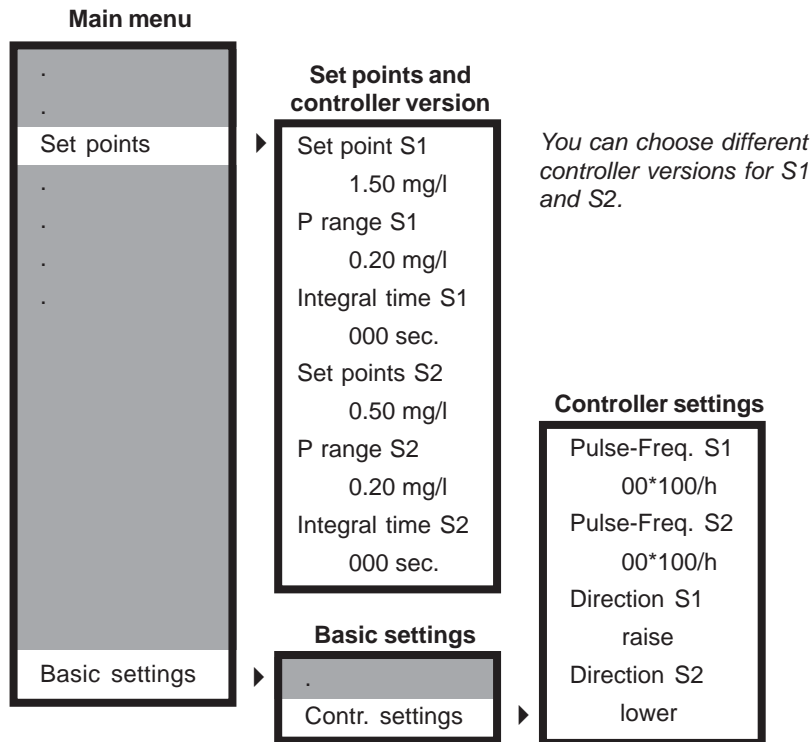

For an impulse-frequency controller you have to set the following parameters:

**1) set points S1 and S2**

S1 refers to relay 1, S2 refers to relay 2.

**2) P range and integral action time for S1 and S2**

Adjust a P range > 0. For a P controller set integral time = 0, for a PI controller set an integral time > 0.


**3) pulse-frequencies for S1 and S2**

Enter the maximum pulse-frequency that corresponds to 100% dosage.

**4) the acting direction for S1 and S2**

Select „raise“ if the dosage raises the measured value.  
Select „lower“ if the dosage lowers the measured value.

## 6.3 P / PI controller as pulse-pause controller

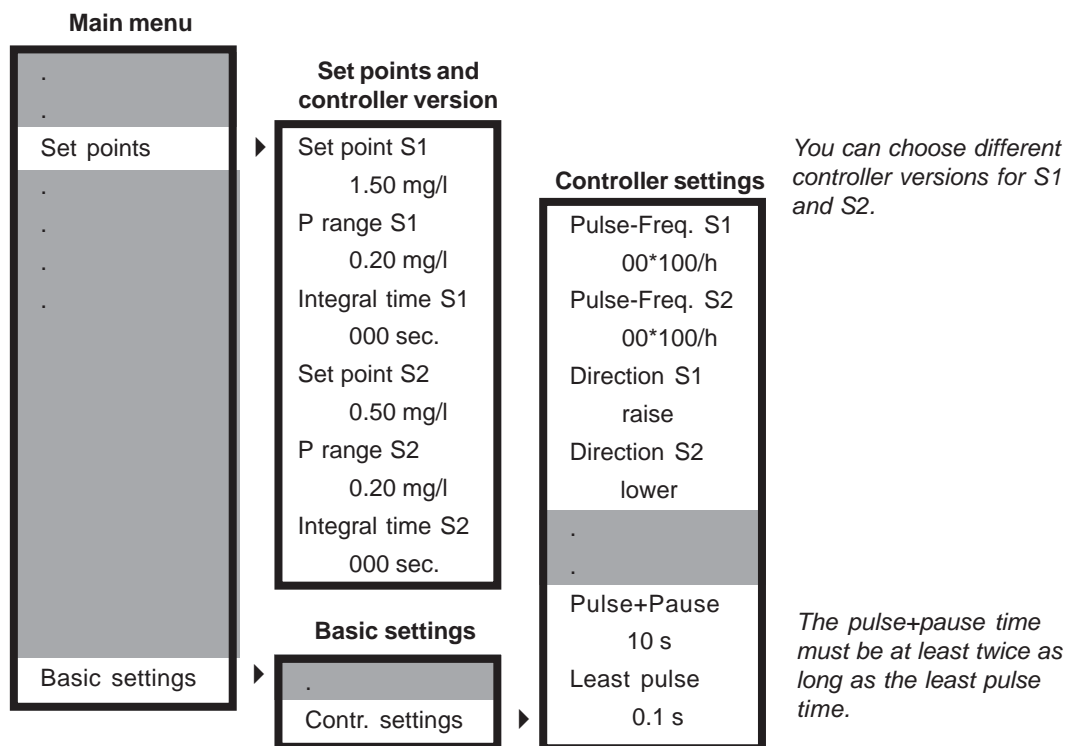

For a pulse-pause controller you have to set the following parameters:

### 1) set points S1 and S2

S1 refers to relay 1, S2 refers to relay 2.

### 2) P range and integral action time

Adjust a P range > 0. For a P controller set integral time = 0, for a PI controller set an integral time > 0.

### 3) pulse-frequencies for S1 and S2

Both frequencies must be set to 00, otherwise the controller will act as an impulse-frequency controller.

### 4) the acting direction for S1 and S2

Select „raise“ if the dosage raises the measured value.  
Select „lower“ if the dosage lowers the measured value.

### 5) pulse+pause time

Define a period of time during which the relay is proportionally to the control deviation ON (pulse) or OFF (pause), respectively.


### 6) least pulse time

Set a minimum pulse time that the relay has to at least remain open to allow the actuator to react.

## 6.4 Activation and deactivation of the controller

You can activate and deactivate the controller without any menu. Press key ▶ to switch between manual operation (controller OFF) and automatic operation (controller ON). The actual operation mode is indicated in the display by MAN or AUTO.

**WARNING** Make sure that the controller is OFF when connecting dosing pumps or other actuators!

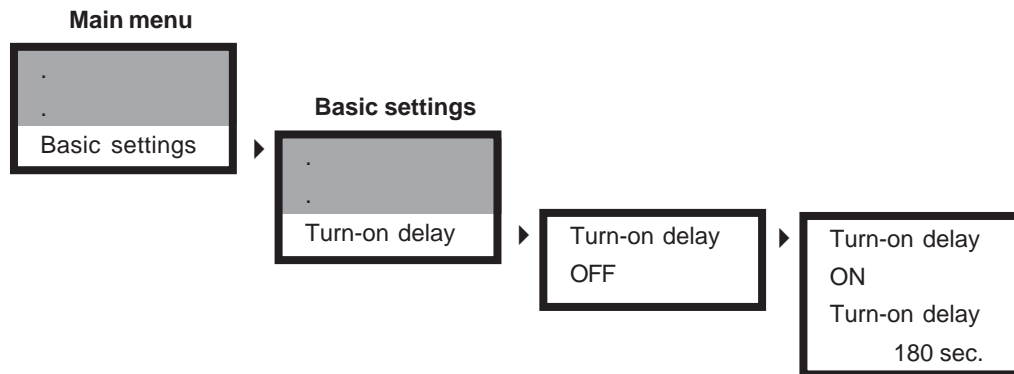

## 6.5 Turn-on delay


Set a delay time which has to pass before the controller is activated after start-up or power interrupt. This allows the measurement to settle and prevents inappropriate dosage of chemicals.

## 6.6 External controller stop


You can activate or deactivate the controller with an external switch by using the digital input. This feature requires no settings or adjustments. If the digital input is short-circuited, the controller stops, and the message „external controller stop“ appears in the display.

**NOTE** This feature is also used as low water indication. The flow monitor is connected to the digital input. However, it can still be used as an external switch - the controller stops as soon as either the flow monitor or the external switch close the digital input.


## 6.7 Manual operation of the relays




- 1) If the controller is ON, switch it OFF with key  $\blacktriangleright$  .  
 Instead of „Auto“ the display shows „Man“.




- 2) Switch to the operation mode of S1 with key  $\blacktriangle$  .  
 The square to the left of S1 starts to flash.




- 3) Switch ON relay 1 with key  $\blacktriangleright$  .  
 The square to the left of S1 gets dark.




- 4) Switch OFF relay 1 again with key  $\blacktriangleright$  .  
 The square gets light.




- 5) Switch to the operation mode of S2 with key  $\blacktriangle$  .  
 The square to the left of S2 starts to flash.



- 6) Switch ON relay 2 with key  $\blacktriangleright$  .  
 The square to the left of S2 gets dark.




- 7) Switch OFF relay 2 again with key  $\blacktriangleright$  .  
 The square gets light.



- 8) Leave the operation mode of relay 2 with key  $\blacktriangle$  .

Both squares appear light, none flashes - You have left the operation mode.



For manual operation you need no menu.

With key  $\blacktriangleright$  you switch OFF the controller.

With key  $\blacktriangle$  you switch between Manual operation <> operation mode S1 <> operation mode S2 <> manual operation.

In the operation mode you can Switch ON and OFF the selected relay with key  $\blacktriangleright$  .


A flashing square indicates that the relay is in operation mode.

A dark square indicates that the relay is switched ON.

A light square indicates that the relay is switched OFF.

**WARNING** If you switch ON a relay it stays ON until you switch it OFF again manually!

## 6.8 Limit values and Alarm

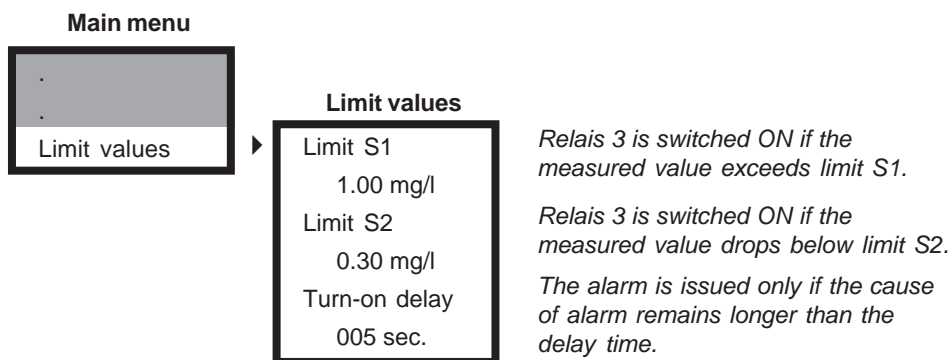

For the alarm, you can adjust two limits: limit 1 is an upper limit. If the measured value exceeds limit 1, an alarm is issued. Limit 2 is a lower limit. The alarm is issued if the measured value drops below limit 2.


In case of alarm the display shows the message „limit 1“ (or 2, respectively), and relay 3 is switched ON. This relay can be used to activate an external horn or lamp.

**NOTE**      **The alarm function is only active when the controller is set on automatic mode. When you switch the controller to MAN, the alarm is extinguished.**

### Turn-on delay

In some applications it happens regularly that the measured value exceeds a limit for a short period of time. To avoid having an alarm issued under these circumstances you can adjust a turn-on delay which has to pass before an alarm is issued. If the turn-on delay time is >0 then the alarm is issued only if the cause of alarm remains longer than the specified turn-on delay time.

## 6.9 Dosage check

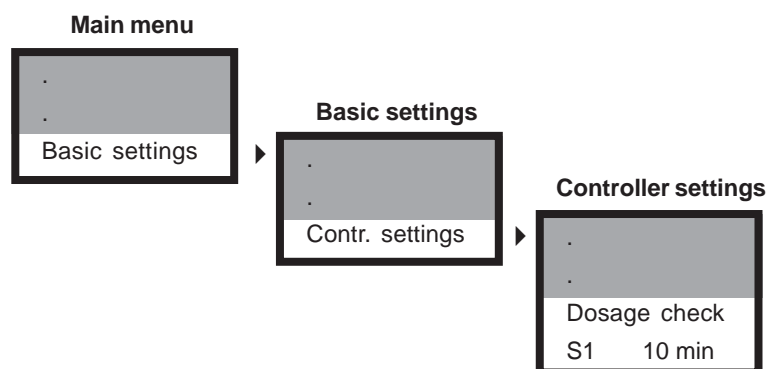

In the basic settings of the controller you can define, how long a controller is supposed to dose with 100% without raising alarm.


If the controller output is 100% for more than the specified time, this is interpreted as an indication of failure, and the instrument issues an alarm and deactivates the controller, thus stopping further dosage.

The dosage check is a safety catch to prevent hazardous chemicals to be set free in case of a defective dosing tube or tube connection.

**NOTE** In case of an alarm due to dosage check, only the controller concerned is deactivated.

**NOTE** If you set the dosage check time to 0 seconds, the dosage check function is deactivated.

## 7. Data output

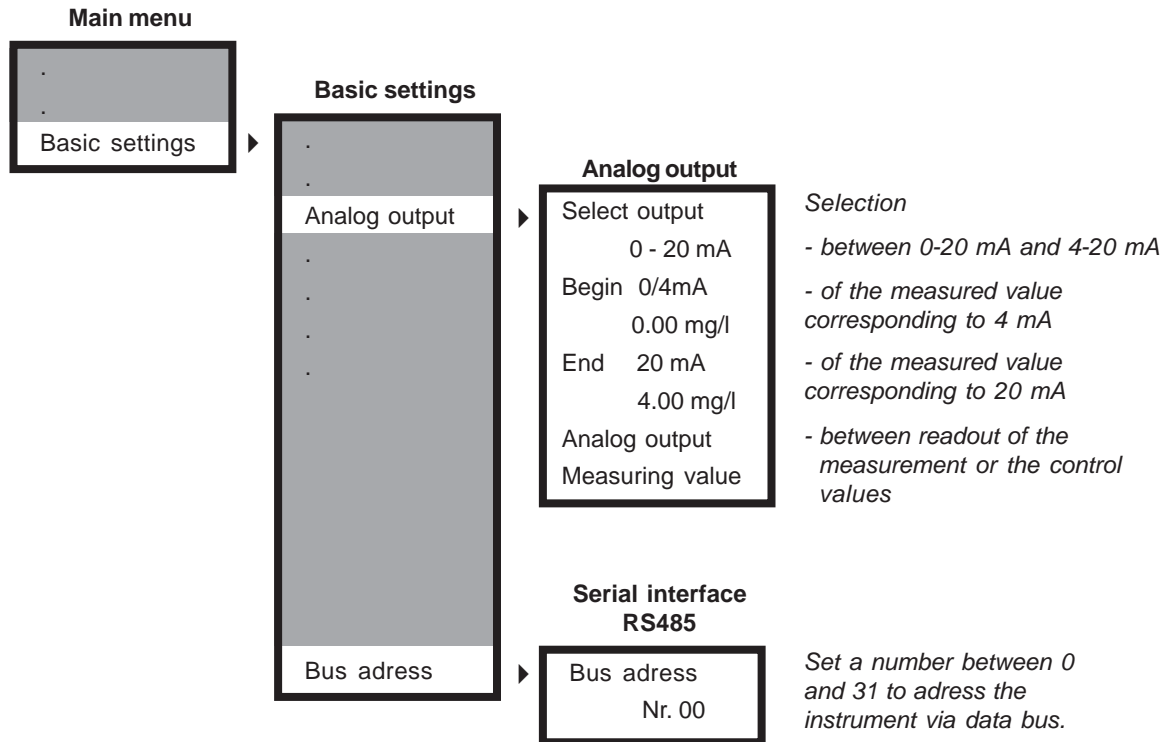

### 7.1 Current output

You can read out the measured values as 0/4-20 mA signals via the current output. With the setting 4-20 mA the resolution is lower, but defective cable connections are immediately evident.

With the parameters Begin and End you define which part of the measuring range you want to read out.

Alternatively you can use the current output as steady-state controller output. In that case assign the current output to the correcting variables S1 bzw. S2.

### 7.2 Serial interface RS485

The instruments are delivered with serial interface RS485 by means of which they can be integrated in a data bus system. Via the interface, all settings, measured and control values as well as any error messages can be read out digitally.

In the leaflet „Information on the RS485“ you will find instructions on the communication and a complete list of the functions available via interface.

## **8. Operation and maintenance**

### **Display contrast**

The display contrast can be adjusted to the actual light conditions by means of a potentiometer. It is indicated in the connection diagram with the word „display“.

### **Cleaning**

The front and the display should not get in touch with organic solutions such as methanol. Never let water get inside the instrument. We suggest to simply use a damp cloth for cleaning.

### **Exchange fuse**

**WARNING! Disconnect the power supply before opening the instrument!**

**ATTENTION Mind that the cable connections to the front are not damaged, broken or torn during the process!**

The instrument has an internal fuse which has to be replaced at need. You will find a spare fuse fixed to the inside of the terminal cover. Information on the fuse can be found in the chapter „Technical data“.

To exchange the fuse, open the front carefully. The fuse is located in the lower right hand side. It is kept in place by a Bayonet lock. Turn the lock to the left until the fuse pops up. Exchange it and fix the new fuse by turning the lock to the right. Put the front back on and fix it tightly.

### **Maintenance of the safety functions**

Regularly check the alarm relay to make sure that in case of failure both the indication by the instrument and the recognition by the superior control (SPS etc.) work reliably.

You can set off the alarm for example by setting limit S1 to a value smaller than the current measured value.

**NOTE Mind that perhaps an alarm delay has been set. Also remember to restore the original settings after the test!**

Regularly check the function of the flow monitor to make sure that in case of a low water situation the sensor gives the signal that leads to the controller stop.

Simulate lack of water by briefly interrupting the water supply. This must lead to a sinking of the flow monitor, and the message „ext. controller stop“ or „no water“ must appear in the display.

---

## **Maintenance of the measurement**

The membrane sensor must be cleaned regularly. Membrane and electrolyte must be exchanged in regular intervals, too. Please refer to the sensor's manual for sensor maintenance.

Mind that the measurement will take some time to repolarise after cleaning or refilling.

Recalibrate if the difference between sensor output and photometric measurement is too large.

**NOTE**        **The instrument checks the calibration data and indicates if a sensor has to be cleaned or electrolyte/membrane exchanged.**

If you have to exchange a sensor, make sure that the replacement sensor is an original Dr. Kuntze product and that it corresponds to the equipment used.

Mind that you have to calibrate whenever you change a sensor - or an instrument!

Regularly clean the flow cell and ensure free movement of the flow monitor.


## **Set-up**

Follow the instructions of this manual. Carry out all steps described. Check both the measured values and the settings before you activate the controller.

## **Disposal:**

For disposal please notice that the instrument contains electrolyte capacitors which have to be disposed separately.

## 9. Service

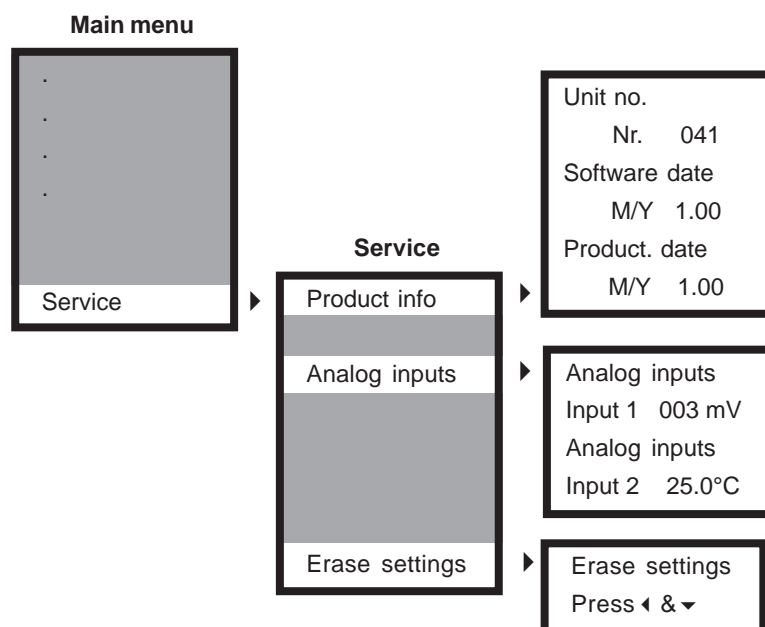

In this menu you will find information which is especially important for any inquiries, updates or problems.

### 9.1 Product info

These figures allow a precise identification of the instrument (hardware and software).

### 9.2 Analog inputs

Here you can see the raw data the instrument obtains from the sensors. They are not influenced by compensations or calibration and offer valuable information in case of problems with the measurement or the instrument.

If you have difficulties interpreting this data, send them to your supplier together with the instrument data - he will know what to do.

### 9.3 Erase settings (reset)

With this function you can erase all customer settings and restore the original at-works data.

The process takes some 30 seconds. When it is finished the display will show the measured value, and the controller will switch off.

## 10. Error messages

<b>Error message</b>	<b>Cause</b>	<b>Measures</b>
Slope error	The slope determined by calibration was higher than 400% or lower than 20 %.	Please check the sensor connection and cable, the flow, and the temperature sensor and settings. Then repeat the calibration. If the error message remains, the sensor has to be cleaned, regenerated, or replaced.
Error input 1	The measuring electrode gives no signal.	Please check the connections, the cable and the sensor for signs of damage.
Error input 2	The temperature sensor gives no signal.	Please check the connections, the cable and the sensor for signs of damage. This message also appears if automatic temperature compensation was selected although no temperature sensor was used or the sensor did not correspond to the settings.
Limit 1 / 2	The measured value exceeded limit 1 (or dropped below limit 2, respectively).	Please check the dosing and readjust the control parameters, if necessary.
Dosage check 1 / 2	Controller 1 (or 2, resp.) gives out a 100% output for more than the defined period of time.	Please check the dosing, especially the feeding tubes and connections. Caution! Carefully check for leaking chemicals!
Ext. controller stop	The digital input has been short-circuited.	This indicates the external controller stop. If issued by the flow monitor, this message indicates „no water“.

---

# Index

## A

Adjustment of the meter .....	17
Adjustments of the controller .....	20
Alarm .....	26
Analog output .....	28

## B

Bus adress .....	28
------------------	----

## C

Calibration .....	18
Code .....	16
Connection diagram .....	11
Connections .....	9
Controller	
Acting direction .....	21
ON/OFF controller .....	20
P controller .....	20
PI controller .....	20
Controller settings	
Impulse-frequency controller .....	22
Pulse-pause controller .....	23
Current output .....	28

## D

Dosing control .....	27
----------------------	----

## E

Erase settings .....	31
Error messages .....	32
External controller stop .....	24

## F

Fuse .....	29
------------	----

## H

Hysteresis .....	21
------------------	----

## I

Impulse-frequency controller .....	22
Interface .....	7

## K

Keys .....	13
------------	----

---

<b>L</b>	
Language .....	16
Limit values .....	26
Low water indication .....	24
<b>M</b>	
Maintenance .....	29
Measuring ranges .....	7
Menu	
Basic settings .....	15
Main menu .....	15
Menu overview .....	15
<b>O</b>	
Operation	
How to adjust parameters .....	14
<b>P</b>	
Password .....	16
Product info .....	31
Protection class .....	8
<b>R</b>	
RC protective circuit .....	9
Relays .....	7
Contact rating .....	8
Manual operation .....	25
Status of the relays .....	13
RS485 .....	28
<b>S</b>	
Serial interface .....	7
Service .....	31
Set points .....	20
Set-up .....	10
Software version .....	5
<b>T</b>	
temperature coefficient .....	19
Temperature compensation .....	19
Temperature sensor .....	19
Turn-on delay	
Alarm .....	26
Controller .....	24

# Customer settings - for reference!

---

## Instrument:

Identification / location: .....

Type: ..... Date of installation .....

Instrument no..... Software version .....

## Measurement:

Averaging:  ON  OFF

## Temperature compensation:

Manual  Automatic

Temperature: ..... °C Correction .....°C

Temperature coefficient .....%/K

## Current output:

0-20mA  4-20mA for:  Meas. value  controller S1  controller S2

Begin: .....

End: .....

## Controller:

Controller S1	Controller S2
Direction: <input type="checkbox"/> raise <input type="checkbox"/> lower	Direction: <input type="checkbox"/> raise <input type="checkbox"/> lower
Set point: .....	Set point: .....
Hysteresys .....	Hysteresys .....
P range .....	P range .....
Integral time .....sek.	Integral time .....sek.
Pulse pause time..... sek.	Pulse pause time ..... sek.
Min. pulse ..... sek.	Min. pulse ..... sek.
Pulse frequency .....*100/h	Pulse frequency .....*100/h
Dosage check ..... min	Dosage check ..... min

## Turn-on delay:

Delay time ..... min.

## Alarm:

Limit S1 ..... Limit S2 .....

Dealy time ..... min.

## Interface RS 485:

Bus adress .....

---